



Human Tissue Factor Activity Kit

Vertrieb:

L O X O GmbH Immunbiologie Biochemie, Produkte und Systeme
Postfach 11 30 69215 Dossenheim
Telefon +49 (0) 62 21 - 86 80 23 **FAX** +49 (0) 62 21 - 86 80 255
E-Mail: info@loxo.de **Internet:** www.loxo.de

Assaypro LLC
30 Triad South Drive
St. Charles, MO 63304
T (636) 447-9175
F (636) 447-9475
www.assaypro.com

Hinweis/Note:

Der Packungsbeileger dient nur als erste Information.
Der relevante Packungsbeileger liegt der Ware bei.

The datasheet is only a first information.
The relevant datasheet is included with the product.

For any questions regarding troubleshooting or performing the assay, please contact our support team at support@assaypro.com.

Thank you for choosing Assaypro.


Symbol Key



Consult instructions for use.

Assay Summary

Add 70 μ l Assay Mix and
add 10 μ l of Standard/ Sample per well.
Incubate at 37°C for 30 minutes.



Add 20 μ l of Factor Xa Substrate per well.



Read at 405 nm every 2 minutes for 20 minutes.

AssaySense Human Tissue Factor (TF) Chromogenic Activity Kit (Two Steps, Lipoprotein)

Catalog No. CT1002b
Sample Insert/Reference Only

Introduction

The transmembrane protein tissue factor (TF) is the physiologic trigger of coagulation in normal hemostasis. TF binds and allosterically activates factor VII (FVII). The TF-FVIIa complex cleaves factor IX and X, leading to thrombin generation (1). TF markedly enhances the ability of FVIIa to cleave both macromolecule and small peptidyl substrates (2, 3). Inducible expression of TF in a variety of pathological conditions, including gram-negative sepsis and acute coronary syndromes, is associated with life-threatening thrombosis (4, 5). In sepsis, TF expression within the vasculature leads to disseminated intravascular coagulation (6). TF also plays important roles in vasculogenesis, metastasis, and tumor-associated angiogenesis (7-9).

Principle of Assay

The AssaySense Human Tissue Factor Chromogenic Activity Kit is developed to determine human TF chromogenic activity in plasma, serum, urine, tissue, and cell culture samples. The assay measures the ability of lipoprotein TF/FVIIa to activate factor X (FX) to factor Xa. The amidolytic activity of the TF/FVIIa complex is quantitated by the amount of FXa produced using a highly specific FXa substrate releasing a yellow para-nitroaniline (pNA) chromophore. The change in absorbance of the pNA at 405 nm is directly proportional to the TF enzymatic activity.

Caution and Warning

- **Prepare all reagents as instructed, prior to running the assay.**
- **Prepare all samples prior to running the assay. The dilution factors for the samples are suggested in this protocol. However, the user should determine the optimal dilution factor.**
- This kit is for research use only.
- The kit should not be used beyond the expiration date.

Reagents

The activity assay kit contains sufficient reagents to perform 100 tests using microplate method.

- **Microplate:** One 96-well polystyrene microplate (12 strips of 8 wells)
- **Sealing Tapes:** Each kit contains 3 precut, pressure sensitive sealing tapes that can be cut to fit the format of the individual assay.
- **Sample Diluent:** 30 ml
- **Assay Diluent:** 20 ml
- **rhTF Standard (Lipoprotein):** 1 vial recombinant human TF lipoprotein
- **Human FVII:** 1 vial
- **Human FX:** 1 vial
- **FXa Substrate:** 2 vials

Storage Condition

- Upon arrival, immediately store components of the kit at recommended temperatures up to the expiration date.
- Store Standard, Factor VII, Factor X, and FXa Substrate at -20°C.
- Store Microplate, Sample Diluent, and Assay Diluent at 2-8°C.
- Unused microplate wells may be returned to the foil pouch and resealed. May be stored for up to 30 days in a vacuum desiccator.
- Opened diluent may be stored for up to 30 days at 2-8°C.

Other Supplies Required

- Microplate reader capable of measuring absorbance at 405 nm.
- Pipettes (1-20 µl, 20-200 µl, 200-1000 µl, and multiple channel).
- Deionized or distilled reagent grade water.
- Incubator (37°C).

Sample Collection, Preparation and Storage

- **Plasma:** Collect plasma using one-tenth volume of 0.1 M sodium citrate as an anticoagulant. Centrifuge samples at 3000 x *g* for 10 minutes, use supernatants, and assay. If necessary, dilute samples using Sample Diluent within the range of 1x – 5x. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles (EDTA or Heparin can also be used as an anticoagulant).
- **Serum:** Samples should be collected into a serum separator tube. After clot formation, centrifuge samples at 3000 x *g* for 10 minutes, remove serum, and assay. If necessary, dilute samples using Sample Diluent

within the range of 1x – 5x. The undiluted samples can be stored at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.

- **Urine:** Collect urine using sample pot. Centrifuge samples at 800 x g for 10 minutes and assay. Store samples at -20°C or below for up to 3 months. Avoid repeated freeze-thaw cycles.
- **Cell Culture Lysates:** The cultured cells are lysed and solubilized with 15 mM octyl-β-D-glucopyranoside at 37°C for 15 minutes. Collect fresh cell lysates and assay. The samples can be stored at -20°C or below for up to 3 months.
- **Tissue:** Extract tissue samples using 50 mM Tris-buffered saline (pH 8.0) with 1% Triton X-100 and centrifuge at 14000 x g for 20 minutes. Collect the supernatant and measure the protein concentration. Dilute the tissue extract 1:4 into Sample Diluent and assay. Freeze the remaining extract at -20°C.

Reagent Preparation

- **Standard Curve:** Reconstitute the rhTF Standard (1500 pM) with 3 ml of reagent grade water to generate a 500 pM standard stock solution. Allow the standard to sit for 10 minutes with gentle agitation prior to making dilutions. Prepare duplicate or triplicate standard points by serially diluting the standard stock solution (500 pM) 1:2 with Sample Diluent to produce 250, 125, 62.5, 31.25, 15.63, and 7.81 pM solutions. Sample Diluent serves as the zero standard (0 pM). Any remaining solution should be frozen at -20°C and used within 30 days.

Standard Point	Dilution	[rhTF] (pM)
P1	1 part Standard (500 pM) + 1 part Sample Diluent	250.0
P2	1 part P1 + 1 part Sample Diluent	125.0
P3	1 part P2 + 1 part Sample Diluent	62.50
P4	1 part P3 + 1 part Sample Diluent	31.25
P5	1 part P4 + 1 part Sample Diluent	15.63
P6	1 part P5 + 1 part Sample Diluent	7.810
P7	Sample Diluent	0.000

- **Human FVII:** Add 1.2 ml reagent grade water.
- **Human FX:** Add 1.2 ml reagent grade water.
- **FXa Substrate:** Add 1.1 ml reagent grade water.

Assay Procedure

- Prepare all reagents, standard solution, and samples as instructed. Bring all reagents to room temperature before use. The assay is performed at

37°C for chromogenic activity assay. Seal the plate with sealing tape at each step.

- Remove excess microplate strips from the plate frame.
- Freshly prepare the desired volume of the Assay Mix by combining the following reagents according to the assay numbers (n) plus one.

<u>Reagents</u>	<u>n=1</u>
Assay Diluent	50 µl
FVII	10 µl
FX	10 µl

- Add 70 µl of the above Assay Mix to each well of the 96-well plate.
- Add 10 µl of rhTF Standard and sample per well of the 96-well plate. Tap plate gently to mix wells.
- Incubate at 37°C for 30 minutes.
- Add 20 µl of FXa Substrate to each well and mix gently. Read the absorbance at 405 nm at zero minutes for background O.D.
- Seal the plate with sealing tape and incubate at 37°C and read the absorbance at 405 nm every 2 minutes for 20 minutes.


Assay Mix	70 µl
TF Standard or Sample	10 µl
<i>37°C, 30 minutes</i>	
FXa Substrate	20 µl
Read the absorbance at 405 nm at zero minutes for background O.D. <i>37°C, Read the absorbance at 405 nm every 2 minutes for 20 minutes.</i>	

Data Analysis

- Calculate the mean value of the duplicate or triplicate for each standard and sample.
- To generate standard curve from the optimal reaction time, plot the graph using the standard concentrations on the x-axis and the corresponding mean 405 nm absorbance on the y-axis. The best-fit line can be determined by regression analysis of the 4-parameter curve.
- Determine the unknown sample concentration from the Standard Curve and multiply the value by the dilution factor.

Standard Curve

- The curve is provided for illustration only. A standard curve should be generated each time the assay is performed.

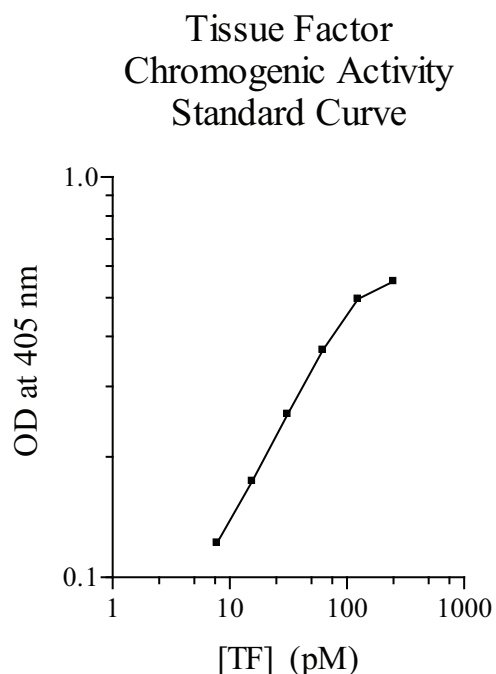

Performance Characteristics

- The minimum detectable dose of TF is typically ~ 7.5 pM.
- This assay recognizes both natural and recombinant human TF.

References

- (1) Ruf, W. and Edgington, T.S. (1994) *FASEB J.* 8:385
- (2) Neuenschwander, P.F. *et al.* (1993) *Thromb. Haemost.* 70: 970
- (3) Morrissey, J.H. (1995) *Thromb. Haemost.* 74:185
- (4) Fuster, V. *et al.* (1996) *Haemostasis* 26:269
- (5) Leatham, E. *et al.* (1995) *Br. Heart. J.* 73:10
- (6) Drake, TA. *et al.* (1993) *Am. J. Pathol.* 142:1
- (7) Carmeliet, P. *et al.* (1996) *Nature* 383:73
- (8) Ruf, W. and Mueller, B.M. (1996) *Curr. Opin. Hematol.* 3:379
- (9) Zhang, Y. *et al.* (1994) *J. Clin. Invest.* 94:1320

Version 7.0